

Continuous Particulate Monitor with X-ray Fluorescence

PX-375

Continuous analysis of
particulate mass and the element
with automatic sampling.



The first step towards prevention of air pollution

In recent years there has been growing concern regarding particulate matter (PM) pollution and its effects on health.

For effective preventative measures, source appointment of PM is extremely important. Therefore, indication of PM elemental concentration is
Newly developed PX-375 enables automatic sampling, continuous online PM quantitative and qualitative analysis and rapid air pollution source

Feature
1

Continuous analysis of PM mass and the elemental concentration by a single unit directly in the field!

- Continuous analysis of PM_{2.5}, PM₁₀ or TSP, mass and the elemental concentration. Sampling and the elemental analysis time are selectable.
- Extremely compact design – 19 inch size and easy installation enables the use of the instrument in scientific laboratories, fixed and mobile air quality monitoring stations (AQMS).
- Ideal for variety of applications: ambient air quality monitoring, indoor air quality control, stationary pollution source appointment, etc.
- Continuous analysis provides you the benefits of reducing labor cost and human errors caused by manual analysis.



Screen image (PC, tablet)



on is to identify pollutant concentration in real ti

also necessary in addition to PM mass concentration.
appointment.

Feature 2

Advanced analysis by world proven technologies.

- Adoption of world proven technologies: X-ray fluorescence & Beta-ray attenuation.
- Compatible with calibration curves evaluated by existing scientific instruments (ICP-MS etc.) for PX-375 calibration.
- Safety features: User is absolutely protected by inter lock. No need to appoint the particular working space and person in charge for the X-ray operation.


Feature 3

HORIBA's newly developed filter tape provides excellent sensitivity and precise performance

- 2 layer non-woven PTFE fabric filter construction prevents passing of PM onto the reverse side.
- Due to the extremely low-impurity concentration, the filter enables ultra low concentration analysis.
- Chemical background of the filter tape is extremely low. Therefore the filter with collected sample could be used for chemical analysis by other scientific analytical instruments. (ICP-MS etc.)

Patents

- USA Patent No.8012231
- CHINA Patent No.ZL200410032415.3
- JAPAN Patent No.4590367



TFH filter

Lowest Detection Limit (Example) (2σ) (ng/m³) (Table 1)

Element	Analysis time (sec.)				
	100	500	1000	5000	10000
S	14.7	6.6	4.6	2.1	1.5
Ti	11.2	5.0	3.5	1.6	1.1
Cr	1.1	0.5	0.3	0.2	0.1
Mn	4.9	2.2	1.6	0.7	0.5
Cu	19.4	8.7	6.1	2.7	1.9
Zn	14.4	6.4	4.5	2.0	1.4
As	0.1	0.0	0.0	0.0	0.0
Se	1.3	0.6	0.4	0.2	0.1
Ag	4.4	2.0	1.4	0.6	0.4
Cd	23.4	10.4	7.4	3.3	2.3
Sn	15.1	6.8	4.8	2.1	1.5
Hg	3.1	1.4	1.0	0.4	0.3
Pb	5.3	2.4	1.7	0.7	0.5

* LDL (σ) is half of the LDL (2σ)

Detectable Elements

(Table 2)

		Detectable Elements																					
H																		He					
Li	Be																	B	C	N	O	F	Ne
Na	Mg																	Al	Si	P	S	Cl	Ar
K	Ca	Sc	Ti	V	Cr	Mn	Fe	Co	Ni	Cu	Zn	Ga	Ge	As	Se	Br	Kr						
Rb	Sr	Y	Zr	Nb	Mo	Tc	Ru	Rh	Pd	Ag	Cd	In	Sn	Sb	Te	I	Xe						
Cs	Ba	Hf	Ta	W	Re	Os	Ir	Pt	Au	Hg	Tl	Pb	Bi	Po	At	Rn							
Fr	Ra		Rf	Ha	Sg	Bh	Hs	Mt	Ds	Rg	Cn	Unt	Fl	Unp	Lv	Uus	Uno						
lanthanoid		La	Ce	Pr	Nd	Pm	Sm	Eu	Gd	Tb	Dy	Ho	Er	Tm	Yb	Lu							
actinoid		Ac	Th	Pa	U	Np	Pu	Am	Cm	Bk	Cf	Es	Fm	Md	No	Lr							

* □—Standard parameters, calibrated by standard calibration materials.

* For measurement of element concentration calibration by standard calibration materials is needed.

* Please contact separately about elements, marked as non-detectable.

Related products

Air Pollution Monitor AP-370 Series



AP-370 Series is used for continuous measurement of several pollutants in ambient air. It is the best trace gas monitor and Nano level particles monitor as well.

- NO_x ● SO_x
- CO ● THC
- O₃

Feature 4

Advanced stationary pollution source appointment by analysis of particulate sample image

Feature 5


User friendly display and operation

- Installed CMOS camera enables observation of collected particulate sample on the filter.
- In addition to particulate mass and elemental concentration analysis, checking the color of particulate sample is possible. Particulate mass concentration, elemental concentration and color – this 3-point approach enables more reliable stationary air pollution source appointment.



- Easy operation and data management by PX-375 data logging PC with original software.
- Convenient trend graph enables user to check particulate mass concentration, element concentration and its correlation at a glance.
- Remote operation* using internet connection will enable user to check status and acquire data without going on site.
*Devices needed for remote access and internet connection should be prepared by customer.
- Operating cost is reduced by omission of the vacuum pump and liquid nitrogen, usually required for X-ray fluorescence detector operation.
- Power distribution function from the main unit for necessary accessories: PC, heater, pump etc.

Air Quality Monitoring Station (AQMS)

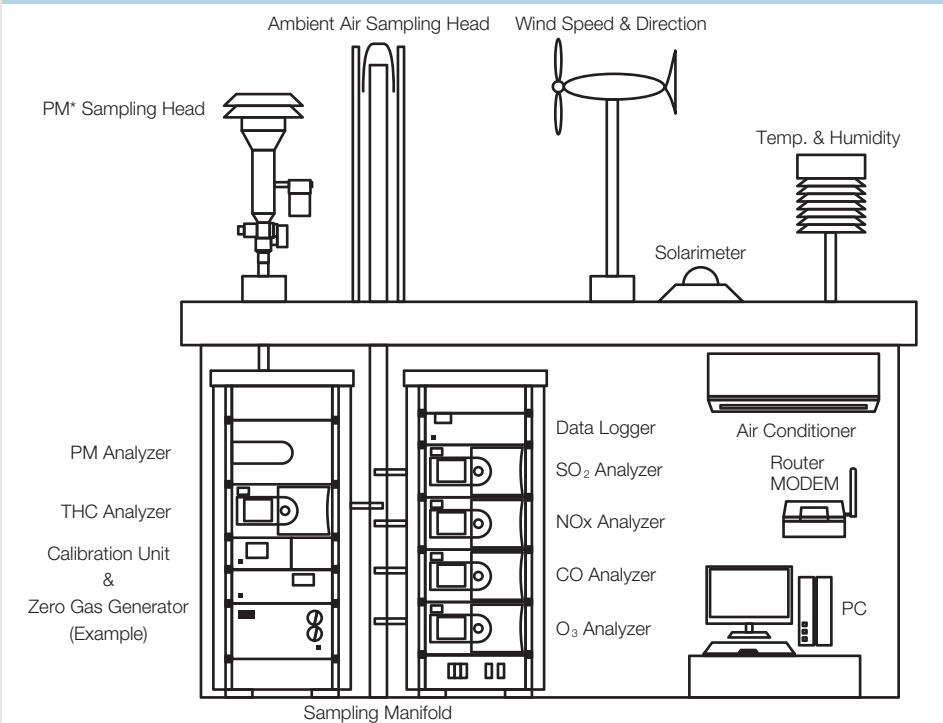

Air Quality Monitoring Station is a facility to monitor wind speed, wind direction and other weather data, concentration of required air pollutants: SO₂, NO_x, CO, O₃, THC and particulate matter during all the year continuously. The measured data could be transferred to the local authorities and other institutions monitoring air pollution in wide region.

Mobile Air Quality Monitoring Stations are available too. Every Monitoring Station is designed and equipped according to customers requests and needs.

*PM: particulate matter

Specifications

Product name	Continuous Particulate Monitor with X-ray Fluorescence
Model	PX-375
Measured object	Particulate matter (PM ₁₀ , PM _{2.5} , TSP)
Measurement content	Particulate mass concentration and element concentration

Common

Flow rate	16.7L/min
Sampling pump	Linear drive system, externally installed
Filter tape	None-woven PTFE fabric filter
Spot tape interval	20/25/50/100mm selectable
Filter tape replacement interval	Approx. 1 month (In case of 100mm spot interval)
Ambient operation temperature	10°C~30°C
Relative humidity	0~80% RH noncondensing
Altitude	1000m or less
Power supply	AC100V~240V ±10%, 50/60Hz±1%
Power consumption	Approx. 400VA
External dimension	430mm(W)×550mm(D)×285mm(H) (without sampling pipe and measurement head)
Weight	Approx. 40kg (Without sampling pipe and measurement head)
Data output	CSV file (Average PM mass and elemental concentration)
External connection	Ethernet™, USB, RS-232C* (option)

*Please consult about communication and instrument composition separately.



Mass analyzer unit

Measurement method	Beta-ray attenuation
PM ₁₀	US EPA Louvered PM ₁₀ Inlet
PM _{2.5}	BGI VSCC™ Cyclone
TSP	TSP Inlet
Measurement range	0~200/500/1000µg/m ³
Repeatability	±2% (against reference foil value)
Span drift	±3% (24hours)
Lowest detection limit (2σ)	±2µg/m ³ (24hours)
Sampling and measurement cycle	0.5/1/2/3/4/6/8/12/24 hours

Element analyzer unit

Measurement method	Energy dispersive X-ray spectroscopy
Detectable elements	See Table 2 "Detectable Elements". Standard parameter is S, Ti, Cr, Mn, Ni, Cu, Zn, Pb, Al, Si, K, Ca, V, Fe, As.
Primary X-ray filter	Automatic switching for light metals/heavy metals
Tube voltage	Automatic switching for 15kV/50kV
Detector	SDD (Silicon Drift Detector)
Sample image	CMOS camera
Lowest detection limit (2σ)	Recommended EPA Method IO 3.3 See Table 1 "Lowest Detection Limit (Example)"
Measurement range	Up to measurement time
Analysis time	1000s (16.6 min) as standard 100 / 200 / 500 / 1000 / 2000 / 5000 / 10000s selectable
Calibration material for X-ray intensity for standard parameter	NIST SRM 2783, other materials (option)
Safety functions for X-ray	Internal lock system
	Key switch
	X-ray indication light

External Dimensions (Unit: mm)

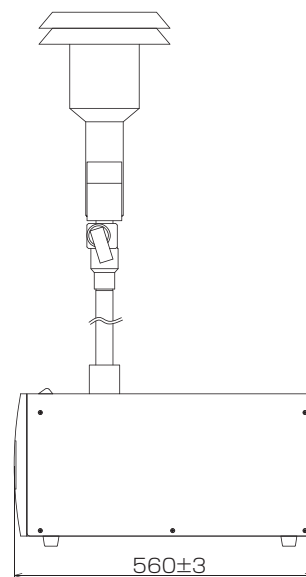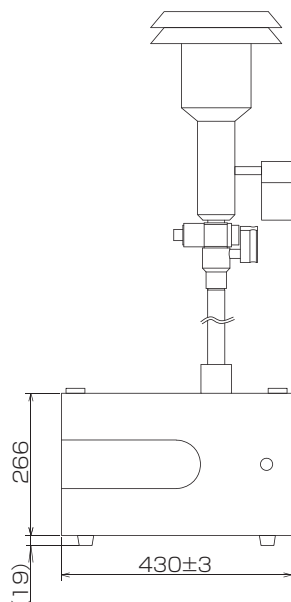

* External dimensions do not include sampling pump, sampling pipe and measurement head.



The HORIBA Group adopts IMS (Integrated Management System) which integrates Quality Management System ISO9001, Environmental Management System ISO14001, and Occupational Health and Safety Management System OHSAS18001. We have now integrated Business Continuity Management System ISO22301 in order to provide our products and services in a stable manner, even in emergencies.



Please read the operation manual before using this product to assure safe and proper handling of the product.

- The specifications, appearance or other aspects of products in this catalog are subject to change without notice.
- Please contact us with enquiries concerning further details on the products in this catalog.
- The color of the actual products may differ from the color pictured in this catalog due to printing limitations.
- It is strictly forbidden to copy the content of this catalog in part or in full.
- The screen displays shown on products in this catalog have been inserted into the photographs through compositing.
- All brand names, product names and service names in this catalog are trademarks or registered trademarks of their respective companies.

<http://www.horiba.com> e-mail: info@horiba.co.jp

HORIBA, Ltd. Japan

Head Office
Unit D, 1F, Building A, Synnex International Park, 1068 West Tianshan Road, Shanghai, 200335, China
Phone: 81 (75) 313-8121 Fax: 81 (75) 321-5725

HORIBA (China) Trading Co., Ltd. China

Shanghai
Unit D, 1F, Building A, Synnex International Park, 1068 West Tianshan Road, Shanghai, 200335, China
Phone: 86 (21) 6289-6060 Fax: 86 (21) 6289-5553
Beijing
12F, Metropolis Tower, No.2, Haidian Dong 3 Street, Beijing, 100080, China
Phone: 86 (10) 8567-9966 Fax: 86 (10) 8567-9066

HORIBA Korea Ltd. Korea

10, Dogok-Ro, 6-Gil, Gangnam-Gu, Seoul-Si, 06259, Korea
Phone: 82 (2) 753-7911 Fax: 82 (2) 756-4972

HORIBA Instruments (Singapore) Pte Ltd. Singapore

3 Changi Business Park Vista #01-01 Akzonobel House, Singapore 486051
Phone: 65 (6) 745-8300 Fax: 65 (6) 745-8155

HORIBA Vietnam Co., Ltd. Vietnam

Unit 6, 10 Floor, CMC Tower, Duy Tan Street, Dich Vong Hau Ward, Cau Giay District, Hanoi, Vietnam
Phone: 84 (4) 3795-8552 Fax: 84 (4) 3795-8553

HORIBA (Thailand) Ltd. Thailand

East Office
850 / 7 Soi Lat Krabang 30 / 5, Lat Krabang Road, Lat Krabang, Bangkok 10520, Thailand
Phone: 66 (0) 2734 4434 Fax: 66 (0) 2734 4438

PT HORIBA Indonesia Indonesia

Jl. Jalur Sutera Blok 20A, No.16-17, Kel. Kunciran, Kec. Pinang Tangerang-15144, Indonesia
Phone: 62 (21) 3044-8525 Fax: 62 (21) 3044-8521

HORIBA India Private Limited India

Delhi
246, Okhla Industrial Estate, Phase 3 New Delhi-110020, India
Phone: 91 (11) 4646-5000 Fax: 91 (11) 4646-5020
Pune

502, 5th Floor, Purushottam Plaza, Baner Road, Baner, Pune-411045 India
Phone: 91 (20) 4076-6000 Fax: 91 (20) 4076-6010

HORIBA Instruments Inc. USA

Bangalore
Kamadhenu, No.17 / 1 - 32, Bannerghatta Road, Audugodi Bangalore-560030 India
Phone: 91 (80) 22210071
Head Office
9755 Research Drive, Irvine, CA 92618, U.S.A.
Phone: 1 (949) 250-4811 Fax: 1 (949) 250-0924
Alvin, TX
5318 W.FM517 Rd, Alvin, TX 77511, U.S.A
Phone: 1 (281) 482- 4334 Fax: 1 (281) 614-0303

HORIBA Instruments Brazil, Ltda. Brazil

Head Office
Rua:Presbitero Plinio Alves de Souza, 645, Loteamento Polo Multivias Baririo Medeiros-Jundiai Sao Paulo CEP 13.212-181 Brazil
Phone: 55 (11) 2923-5400 Fax: 55 (11) 2923-5490

HORIBA France Sarl France

12, Av des Tropiques Hightec Sud, F-91955 Les Ulis, France
Phone: 33 (1) 69-29-96-23 Fax: 33 (1) 69-29-95-77

HORIBA UK Limited UK

Northampton
Kyoto Close Moulton Park, Northampton NN3 6FL, UK
Phone: 44 (1604) 542-500 Fax: 44 (1604) 542-699

HORIBA Europe GmbH Germany

Head Office
Hans-Mess-Str.6 D-61440 Oberursel Germany
Phone: 49 (6172) 1396-0 Fax: 49 (6172) 1373-85
Leichlingen
Julius-kronenberg Str.9 D-42799 Leichlingen Germany
Phone: 49 (2175) 8978-0 Fax: 49 (2175) 8978-50

HORIBA Czech Czech

Prumyslova 1306 / 7, CZ-10200, Praha 10, Czech Republic
Phone: 420 (2) 460-392-65

HORIBA (Austria) GmbH Austria

Kaplanstrasse 5 A-3430 Tulln, Austria
Phone: 43 (2272) 65225 Fax: 43 (2272) 65230